

# SCIENTIFIC POSTER PRESENTATION AWARD

## Evaluation of Extracorporeal Blood Heat Exchanger Devices

Robert Barthelemy, MD, Nicolas Chauveau, MS

Division of Experimental Surgery, Rangueil Hospital  
and National Institute for Health and Medical Research, Hotel Dieu Hospital  
Toulouse, France

**Keywords:** Extracorporeal circulation, heat exchanger, efficiency

---

### Abstract

An accurate and easy to use test circuit has been developed, for performance evaluation of heat exchangers used in cardiac surgery during extracorporeal circulation. The water part of the heat exchanger is fixed at a flow rate of 15 l/min and at a temperature of 40°C. For blood, the flow rate is varied from 1 to 6 l/min and the temperature is 30°C. The use of a very precise thermometer (precision 0.01°C) and of a microcomputer permits one to obtain the efficiency with very good reproducibility. The results obtained show a real improvement in the efficiency of the new extracorporeal blood heat exchanger devices.

---

### Introduction

A heat exchanger is a system used in extracorporeal circulation (ECC), that lowers the patient blood temperature during the ECC and increases it at the end of the operation.

It consists of a water circuit separated from the blood circuit by the surface of the heat exchanger, (Figure 1) TWO represents temperature of the water out, TWI represents temperature of the water in, and TBI is the temperature of blood in, TBO is the temperature of the blood out.

### FIGURE 1: Schematic of the Heat Exchanger

Many heat exchangers are available with a wide range of efficiency. The principle behind heat exchangers has been defined by Galetti (1), Pierce (2), Reed (3), and Riley (4).

New heat exchangers have been recently developed and have been tested in order to evaluate their relative performance.

*Address correspondence to: Robert Barthelemy, MD, Division of Experimental Surgery, Rangueil Hospital, Chemin du Vallon, 31054 Toulouse Cedex, France.*

The main parameters that must be taken into account are:

- the material (metal or plastic)
- the thickness of the heat conductor
- the thermal conductance in cal/sec/cm/°C
- the heat conductor area
- the heat lost to environment
- the priming volume
- the mean blood path thickness
- the blood and water path resistances
- the effect of water flow variation on efficiency
- the efficiency of the heat exchanger

To be precise, a comparison must take into account at least all these parameters. The evolution of ECC has led to the development of different kinds of heat exchanger devices, integral to the oxygenator or otherwise. In such conditions, it is difficult even sometimes impossible to isolate the heat exchanger for proper tests.

One very important parameter that can be tested in all cases is the heat transfer efficiency which is defined as:

$$\text{Efficiency} = (TBI - TBO) / (TBI - TWI)$$

TBI - blood input temperature

TBO - blood output temperature

TWI - water input temperature

---

### Material and Methods

For the measurements (Figure 2), the flow rate in the water circuit is fixed to 15 l/min and varied from 1 to 6 l/min in the blood circuit. Thus, it is through this protocol that the effect of flow rate variation in the blood circuit was tested.

The three temperatures are measured with Yellow Springs Instruments (YSI) thermistors (a), matched in order to be reliable with 0.01°C. To ensure comparable values, the same electronics were used to measure the three temperatures. A multiplexer is used to connect the probe to the electronics, thus ensuring the same measurement error is done on each temperature signal. A Cole-Parmer (b) portable thermistor

a. Yellow Springs Instruments.

b. Model 8502-16, Cole-Parmer.


c. Apple II, Apple Computers, Inc.

thermometer (Model 8502-16), with three input channels and one analog output was employed. Because there is only one analog output, the signal corresponding to this output is the one displayed by the liquid-crystal display of the device. In order to change the channel displayed you have to change the analog channel input.

The thermometer is coupled to an Apple (c) microcomputer, in order to achieve more easily the calculation of the efficiency. A 10 bit analog-to-digital converter is used with a full scale 0.41 volt corresponding to a range of 41°C for the analog output of the device.

In order to maintain absolute reliability between all heat exchangers, water was utilized on both sides of the heat exchanger instead of water to blood. Since the conditions are the same for all the heat exchangers tested, the relative values are the basis for comparison, and not absolute values.

**FIGURE 2: The Test Circuit**

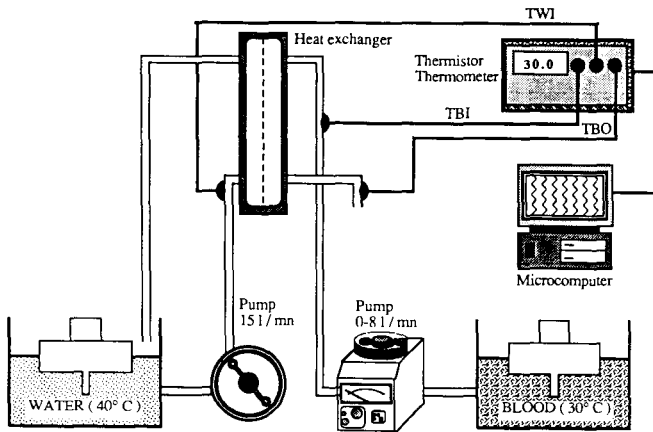

**EFFICIENCY MEASUREMENT SYSTEM**

The test circuit includes (Figure 2):

- a stand for tubing, valves, mounting of the heat exchanger to be tested.
- a 100 liter tank of water regulated at 40°C for the water part of the heat exchanger
- a 60 liter tank of water regulated at 30°C for the blood part of the heat exchanger
- four thermistor thermometer probes with display and analog output
- an Apple II microcomputer for the calculation and the display of the procedure.

During the test procedure, the water pump flow rate is fixed to 15 l/min for the water part, and the water pump (blood) is varied from 1 to 6 l/min.

The measurement procedure is as follows: the temperature of the inlet water as measured by the thermistor thermometer is displayed and validated by the user on the microcomputer keyboard. Then the same process is repeated for the water (blood) inlet temperature. The display of the outlet water (blood) temperature is recorded in real time and the efficiency of heat exchange is obtained by calculator.


Currently, only static efficiency in a steady state position is

being measured. This is accomplished in the following manner: TWI, TBI and the water (blood) flow rate are selected and allowed to stabilize before the measurement begins. In this way, the time response of the heat exchanger to varying blood flow rates can be taken into account. The efficiency is measured for different flow rates varying from 2 to 6 l/min. The advantage of our measurement system is its great precision and stability.


**Results**

The results show that in the normal range of blood flow rate which is from 4 to 6 l/min, the heat exchangers of the previous generation (Figure 3) present lower performances than the ones of the new generation (Figure 4). In addition, the new ones have closer performances than before.

**FIGURE 3: Heat Exchangers Tested in 1975**

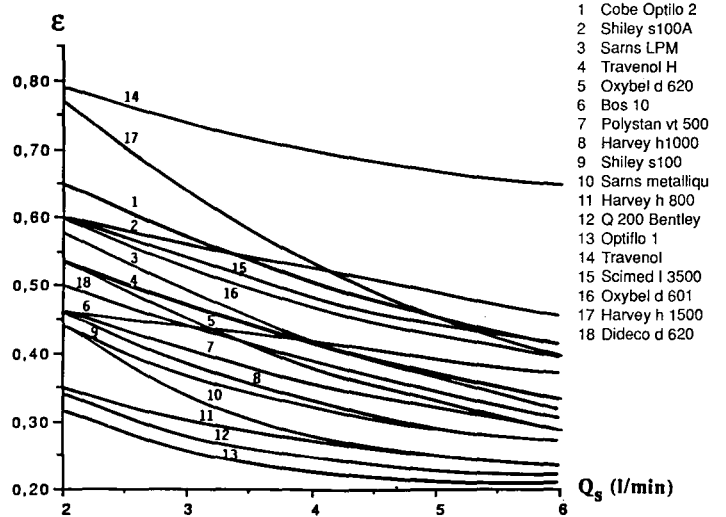

**FIGURE 4: Heat Exchangers Tested Since 1989**

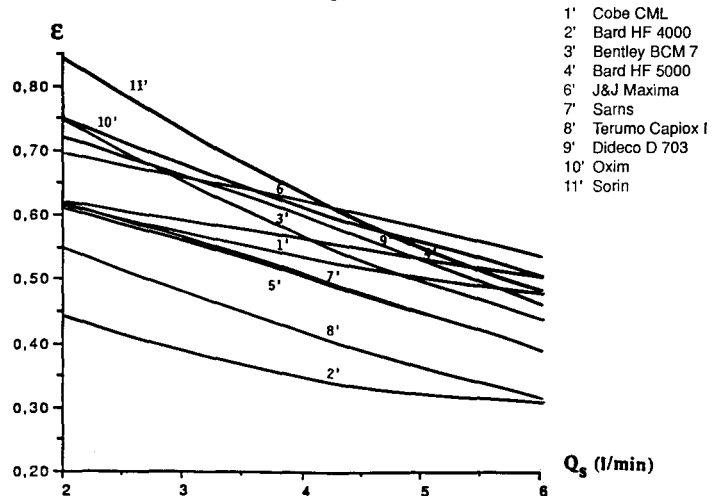

**Conclusion**

Great improvements have been made in the design of heat exchangers, such that they now present values which are quite similar in efficiency. We have now an operational test circuit,

which is easy to use and able to test all the new heat exchangers, with ease, accuracy and good reproducibility.

#### References

---

1. Galetti P, Brecher G. Heart-Lung Bypass: Principles and Techniques of Extra-Corporeal Circulation. New York: Grune and Stratton; 1962: 200-206.
2. Pierce EC. A simplified heat exchanger for perfusion hypothermia: *Arch. Surg.* 1962; 84: 329-333.
3. Lawrence E., Wilson D., Hanks E., Morris A clinical in vivo comparison of a non disposable external, and an integral disposable heat exchanger: *JECT.* 1977; 9(3): 67-69.
4. Riley J B, Winn B. In vitro analysis of extracorporeal blood heat exchange devices: *JECT.* 1977; 9(3): 134-144.